

Comparison of BACTEC 9120 and Conventional Blood Culture Systems for Isolation of Microorganisms from Blood and Other Sterile Body Fluids

Said Maham¹, Fariba Shirvani¹, Mana Hadipour Jahromi¹,
Fateme Fallah¹, Seid Sajad Razavi², Ali Nikfarjam³ and Mohammad Rahbar^{4,5}

¹Pediatric Infections Research Centre, Mofid Children Hospital,
Shaheed Beheshti University of Medical Sciences and Health Services

²Department of Pediatric Mofid Children Hospital,
Shaheed Beheshti University of Medical Sciences and Health Services

³Ministry of Health and Medical Education

⁴Department of Microbiology, Iranian Health Reference Laboratory,
Ministry of Health and 5-Medical Education, Tehran, Iran.

⁵Antimicrobial Resistance Research Center, Tehran University of Medical Sciences, Tehran, Iran.

(Received: 12 April 2012; accepted: 30 May 2012)

Bloodstream infectious diseases are prevalent in children and adults. Rapid and accurate diagnosis of bloodstream infections primary based on conventional culture results, which saves time and prevents empiric treatment. The aim of this study was to compare the results of BACTEC 9120 and conventional culture systems, on blood specimens collected from three university affiliated hospitals in Tehran, Iran. BACTEC 9120 and conventional methods were used for isolation of microorganism from specimens including blood and other body fluid samples collected from patients hospitalized in the selected hospitals during the study period, from April to June 2009. Time for positive and negative results and hospital charge were estimated for the two culture methods. In total 747 specimens were possessed by BACTEC 9120 systems and 787 by conventional method. Patients aged between 3 days and 8 years old, (mean 11.4 ± 21.9 years); 52% of patients were male and 48% female; Out of 747 specimens were possessed by BACTEC 9120 system, 26% (196/747) and from 787 specimens cultured by conventional method 5% (49/787) were positive ($p < 0.05$). Hospital stay was 13.8 ± 12.9 days in BACTEC 9120 and 17.9 ± 14.9 days in Conventional method, ($p < 0.05$) respectively. Time for positivity by BACTEC system was 3.8 ± 1.1 Days and 5.9 ± 2.5 days in conventional method. ($p < 0.05$), treatment response showed 1.8 day earlier result in patients that their specimens were processed by BACTEC 9120 system. Death rate in BACTEC 9120 method was 6% and 11% in Conventional method. ($p > 0.05$). In conclusion implementation of BACTEC system for microbiologic detection of pathogens decreases the admission time and early diagnosis and treatment results are cost effective for patient management and prevention of antibiotic resistance.

Key words: Blood culture system, Sterile body fluids.

* To whom all correspondence should be addressed.
E-mail: shirvani@sbmu.ac.ir;
fariba_shirvani@yahoo.com

Bloodstream infections are one of the most important problems among infectious disease. Proper antibiotic treatment of bloodstream infections initially based on isolation, identification and performance of susceptibility testing on microorganisms isolated from blood cultures¹. In spite of recent improvements such as molecular procedures for microbiological diagnosis, blood

culture still is the most reliable method for diagnosis of bloodstream infections. Conventional diagnostic methods including manual systems and culture media are available in majority microbiology laboratories. In traditional methods blood culture bottles are inoculated with blood and usually incubated for seven days. Subculture on solid media, isolation and susceptibility testing in these methods are time consuming, process. High number of requested cultures and necessity of rapid bacteriologic results calls for a novel bacteriologic diagnostic apparatus with higher capacity and speed, for processing the accuracy and precision of results³. BACTEC system can be used not only in blood cultures but also in other sterile body fluids with low volume and few identifiable microorganisms⁴. Several blood culture systems such as Bactec Ped Plus are used for isolation microorganisms from blood specimens in children⁵. This system also helps distinguishing bacterial pathogens from contaminant organisms as the source of infectious diseases⁶.

In this study we compared the traditional culture systems with the novel BACTEC system to evaluate the efficacy of the BACTEC blood culture system in sterile body fluids.

MATERIALS AND METHODS

All patients admitted in Mofid, Logman, and Talegani Hospital from April-June 2009, whom blood and other body fluid specimens had been obtained, were included in this study. Patients hospitalized for less than 2 days were excluded. The Bacteriologic Apparatus was BACTEC 9120 (Becton Dickinson Diagnostic Instrument System USA) continuous monitoring Blood culturing instrument which accommodates 120 test bottles. BATEC 9000 systems feature the unique Bactec 9000 fluorescent sensor technology that allows for fully automated, walk away testing using a continuous monitoring instrument that agitates and incubates BACTEC/F blood culture bottles resulting in earlier detection of positive cultures. It provides advanced algorithms for individual bottle types for special circumstances as low blood volume, pediatric or other sterile fluid specimens. The metabolic precursors labeled with C¹⁴ are included in the broth medium and with

microorganism's growth; they liberate ¹⁴CO₂ in the broth which diffuses in the bottle headspace atmosphere. A "growth index" exceeding a predefined threshold is considered evidence of microbial growth and prompts a gram stain and subculture of the specimen- broth mixture⁷. Eight types of vials are available for culture; at least one milliliter of blood or other body fluids (infused in bottles and specimens are detected at least after 7 hours to 5-7 days. Routine blood cultures in parallel with Bactec was performed. Organisms isolated from blood cultures and other body fluids were identified by conventional laboratory methods. Demographic data and medical records were abstracts patient, s files. Assessment of clinical significance was based on symptoms and positive numbers of bottle cultures. The results were recorded in SPSS 18.2, T test and Chi Square was done for quantitative and qualitative data and Kaplan Mayer Graph was drawn for survival data.

RESULTS

A total of 747 specimens were tested by the BACTEC 9120 and 787 specimens by traditional method. Patients' age range was from 3 days to 89 years, (mean, 11.4±21.9 years), 52% of the specimens were from males. 195 out of 747 of specimens tested by th BACTEC 9120e (26%)? and 44 of 787 specimens (5%) subcultured on conventional agar plates were positive, (P<0.05, table 1). , Result of cultures by different methods, different sites and from different centers are shown in tables 2 and 3. There was a significant difference in the duration of hospital stay in the 2 group of patients, by using the BACTEC 9120 Method. Mean time hospitalization was 13.8 ± 12.9 days and in patients in whom cultures were done by the routine method it was 17.9 ± 14.9 days (p<0.05). The duration until response to treatment was 3.8 ± 1.1 days wit BACTEC 9120h and 5.9 ± 2.5 days with the routine method, (p<0.05). Correlation between culture results and time of discharge patients in two methods shows significant longer time in routine method (B under-standardized Coefficient =1.8, p<0.001). Figure 1 and 2 shows the time of positive and negative culture results in Bactec and Routine culture methods.

Table 1. The result of different microorganisms isolated in BACTEC system and conventional culture method

Microorganism	BACTEC n=747	Conventional n=787	p-Value
Coagulase-Negative staphylococci	58 (7.76%)	11 (1.4%)	<0.001
<i>E-coli</i>	27 (3.61%)	10 (1.27%)	0.003
<i>Staphylococcus aureus</i>	12 (1.61%)	9 (1.14%)	0.44
<i>Enterococcus faecalis</i>	9 (1.2%)	5 (0.64%)	0.24
<i>klebsiella pneumoniae</i>	8 (1.07%)	3 (0.38%)	0.11
<i>Candida albicans</i>	7 (0.94%)	1 (0.13%)	0.03
<i>Citrobacter freundii</i>	7 (0.94%)	1 (0.13%)	0.03
<i>Streptococcus viridans</i>	7 (0.94%)	1 (0.13%)	0.03
<i>Enterobacter aerogenes</i>	6 (0.8%)	1 (0.13%)	0.06
<i>Proteus vulgaris</i>	6 (0.8%)	1 (0.13%)	0.06
<i>Stenotrophomonas maltophilia</i>	6 (0.8%)	1 (0.13%)	0.06
<i>Acinobacter baumannii</i>	6 (0.8%)	0 (0%)	0.01
<i>Streptococcus pneumoniae</i>	6 (0.8%)	0 (0%)	0.01
<i>Proteus mirabilis</i>	5 (0.67%)	0 (0%)	0.03
<i>Pseudomonas aeruginosa</i>	5 (0.67%)	0 (0%)	0.03
<i>Burkholderia cepacia</i>	4 (0.54%)	0 (0%)	0.06
Bacteroides spp.	3 (0.4%)	0 (0%)	0.12
<i>Hafnia alvei</i>	3 (0.4%)	0 (0%)	0.12
<i>Moraxella catharralis</i>	3 (0.4%)	0 (0%)	0.12
<i>Providencia stuarti</i>	2 (0.27%)	0 (0%)	0.24
<i>Enterobacter cloaceae</i>	1 (0.13%)	0 (0%)	0.49
Group D streptococci	1 (0.13%)	0 (0%)	0.49
<i>Edwardsiella tarda</i>	1 (0.13%)	0 (0%)	0.49
Beta hemolytic non-group A Streptococci	1 (0.13%)	0 (0%)	0.49
Peptostreptococcus sp	1 (0.13%)	0 (0%)	0.49
Peptococci	1 (0.13%)	0 (0%)	0.49
Total positive cultures	196 (26.24%)	44 (5.59%)	<0.001

Table 2. Frequency of different specimens

Specimen	BACTEC	Routine
Blood	665(89%)	645(81%)
CSF	40(5%)	71(9%)
Tracheal aspiration	10(1%)	2
Peritoneal dialysis fluid	10(1%)	0
Pleura	7(0.09%)	4(0.05%)
Synovium	4(0.05%)	0
Shunt	3(0.04%)	0
Cyst	3(0.04%)	0
Ascite fluid	2(0.02%)	37(5%)
Peritoan	1(0.01%)	7(0.08%)
Bone Marrow	1(0.01%)	0
Wound	1(0.01%)	0
Throat	0	21(2%)
Total	747	787

Table 3. Frequency of samples from different wards

Ward	BACTEC	Routine
Gynecology	147(20%)	0
Cardiology	86(11%)	11(1%)
ICU	84(11%)	17(2%)
Othopedics	72(9%)	6(0.07%)
hematology	66(8%)	56(7%)
NICU	56(7%)	119(15%)
Surgery	47(6%)	41(5%)
Infectious disease	47(6%)	61(7%)
Gastrointestinal	35(4%)	74(9%)
Emergency	25(3%)	166(21%)
nephrology	22(2%)	35(4%)
neonatal	15(2%)	129(16%)
Bone Marrow Transplant	13(1%)	43(5%)
Internal	9(1%)	1(0.01%)
Neurology	9(1%)	12(2%)
PICU	5(0.06%)	6(0.07%)
pediatric	4(0.05%)	0
CCU	4(0.05%)	0
Endocrinology	1(0.01%)	10(1%)
Total	747	787

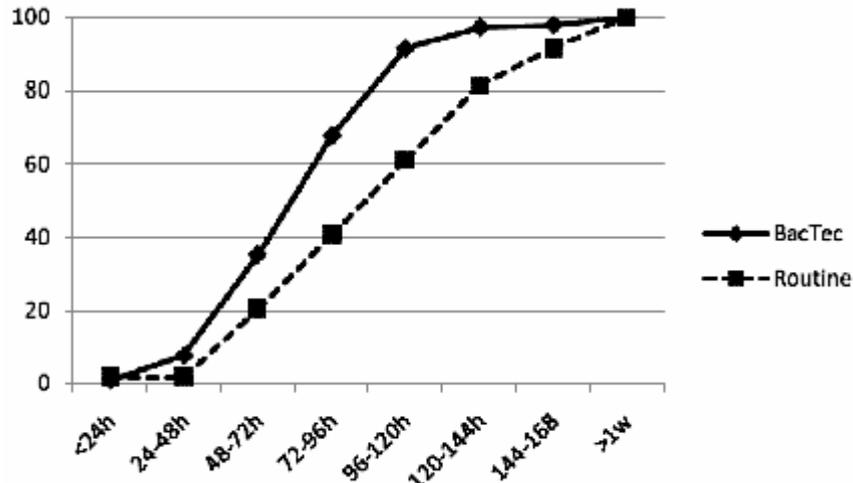


Fig. 1. Time needed for positive culture results in conventional and Bactec cultures

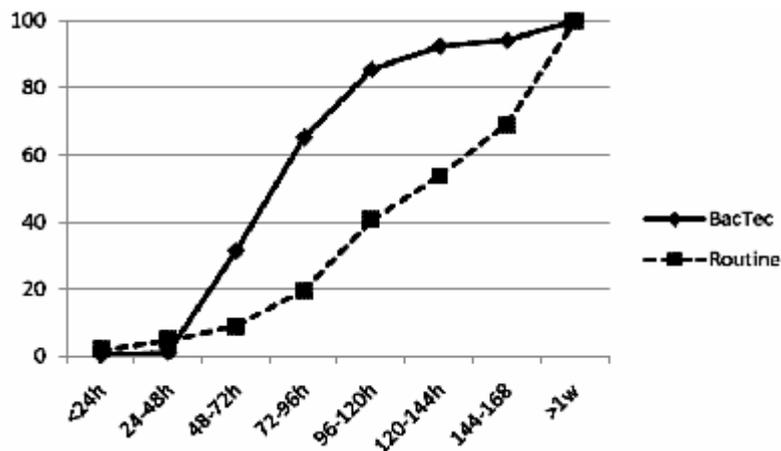


Fig. 2. Time needed for negative culture results in conventional and Bactec cultures

DISCUSSION

Blood cultures are the most important microbiologic laboratory test and recently many "new technology" automated blood culture systems are introduced and in some centers they are used for instantaneous diagnosis on blood samples collected from patients⁸. The BACTEC 9120 blood culture system received 510k FDA clearance in 1992, this is a CMBCS (Continuous Monitoring Blood Culture System)⁷. In this study blood and other sterile body fluids cultures showed significantly more pathogenic microorganisms than traditional culture methods. Similar results from

studies in Iran show that utilizing the BACTEC system reduces the time of admission with faster responses to therapy⁹. Resin containing media may improve the yield of BACTEC radiometric system which by using resin media, provided for recovery of clinically significant organisms equivalent to those recovered by the isolator^{10,11}, lowering the contamination rate helps in detection of bacteria in sterile body fluids, with positive results for better antibiotic selection. We couldn't detect contamination due to lack of sufficient data in our patients records¹². BACTEC 9120 System shows its role in detection of factitious organisms such as *Brucella*, *Micobacteria* and *Kingella Kinga* in

CSF, peritoneal fluid, intraorbital and intraarticular space and for unusual pathogen such as *C.upsaliensis* from blood culture of leukemic patients¹³⁻¹⁶ and anaerobic organisms in blood cultures¹⁷.

Hospital charge is another important issue in developing countries and patient load waiting for admission and extreme need for time saving is an important priority, each day of admission in Mofid Children's Hospital incurs a cost of at least 261000 Rials equivalent to 20.7 dollars. The time needed for positive response in BACTEC 9120 system was 2 days less than for the conventional method in this study. Choosing an antibiotic based on bacteriologic results, prevents antibiotic resistance, accordingly the study showed high correlation co efficiency by regression analysis between time of laboratory results and mean admission time i.e. each day of earlier report may result in 1.8 days of earlier discharge. Other studies also showed a reduction in the duration of hospitalization and prompt treatment, together with appropriate antibiotic selection thus lowering the hospital charges¹⁸. Moreover, using 5 days BACTEC 9120 Protocol by automated culture system reduces the laboratory workload¹⁹.

In conclusion using automated systems for isolation of microorganisms from sterile body fluid cultures is cost effective, reduces inappropriate antibiotic therapy, prevents antibiotic resistance and saves lives by reducing morbidity and hospital stay of children hospitalized in private and public hospitals.

ACKNOWLEDGEMENTS

We thank Dr Masomeh Navidnia, Mr Malekan and Mrs Zari Golinagad for their great assistance in undertaking the multiple tasks of performing the different procedures required for this study.

REFERENCES

1. Esteban J, Fernandez-Roblas R, Cabria F, Soriano F, Usefulness of the BACTEC MYCO/F lytic system for detection of mycobacteremia in a clinical microbiology laboratory. *Journal of Microbiological Methods* 2000; **40**: 63-66.
2. Ryan M, Murray PR. Historical evaluation of automated blood culture systems. *Diagnostic Microbiology and infectious Diseases* 2000; **38**(4): 223-6.
3. Cetin ES, Kaga S, Demirci M, Aridagon BC, Comparison of the Bactec blood culture system versus Conventional methods for Culture of normally sterile body fluids, *advances in therapy* 2007; **24**(6):1271-77.
4. Lupetti A, Balnini S, Castagn B., Copria A.L, Nibbering P.H, Raid identification and antimicrobial susceptibility profiling of gram positive cocci in blood culture with the Vitek Z system. *Eur J Clin Microbiol infect Dis.* 2010; **29**: 89-95.
5. Welby P.L, Zusay T.M, Storch G.A, Comparison of the Bactec Peds plus Pediatric Blood culture vial with Roche Pediatric Septi-check for blood cultures from pediatric patients *Journal of Clinical Microbiology.* 1992; **30**(5):1361-62.
6. Hughes J.C, Vetter E.A, Patel R, Schleck C.D, Harmsen S, Turgeant L.T, Cockerill F.R, Culture with Bactec Ped Plus F bottle compared with conventional methods for detection of bacteria in synovial fluid *J of Clin Micro.*, 2001; **44**: 68-71.
7. Reimer L.G, Wilson M.L, Weinstein M.P. Update on detection of bacteremia and fungemia, *Clinical microbiology reviews*, 1997; **10**(3): 444-65.
8. Sanches A.M, Roman S, Fiola Y, Lenton P, Hording G, Continuous quality improvement for introduction of Automated blood culture instrument. *Journal of Clinical Microbiology*, 1995; **33**(5):1185-91.
9. Barati M, Norbachsh S, Bactec culture system, an effective method for isolation of microorganisms from sterile sites of body. *Journal of Medical college, Tehran Medical Sciences University.* 1387; **66**(5): 305-10.
10. Brannon P, klehn TE. Clinical comparison of lysis- centrifugation and radiometric resin systems for blood culture. *J Clin Microbiol.* 1986; **24**: 886-7.
11. Courcol R.J, Dourocher A.V, Oclvallez M.R, Fruchart A, Martin G.R. Routine evaluation of Bactec NR-16A and NR-17A media. *J Clin Microbiol.* 1988; **26**:1619-22
12. Hughes J.C, Vetler E.A, Patel R, Schleck C.D, Haarmen S, Turgeant L.T, Cockerill F.R. Culture with Bactec Peds Plus/F Battle compared with Conventional Method for detection of Bacteria in Synovial fluid. *J of Clin Micro.* 2001; **39**(12): 4468-71
13. Akam F.Z, Yayli G, Uskun E, Kaya O, Demic C, Evaluation of the Bactec microbial detection

- system for culturing miscellaneous sterile body fluids. *Research in Microbiology* 2006; **157**(5): 433-6.
14. Carnahan A.M , Beadling J , Watsky D, Ford N .Detection of *Campylobacter Upsaliensis* from a Blood culture by using a Bact/Alert system.*Journal of Clinical Microbiology*. 1994; **32**(10): 2598-99.
 15. Yagupsky P, Dagan R , Howard C.W, Einhorn M, Kassis I, Simi . High prevalence of *Kingella Kingae* in joint fluid from children with Septic Arthritis revealed by the Bactec blood culture system. *Journal of Clinical Microbiology*. 1992; **30**(5): 1278-81.
 16. Brunello F ,Favari F, Fontana R.Comparison of MB/Bact and Bactec 460 TB systems for recovery of Mycobacteria from various clinical specimens. *Journal of Clinical Microbiology*., 1999; **37**(4): 1206-9.
 17. Bannister E.R, Woods G.L. Evaluation of routine anaerobic blood culture in Bact/Alert blood culture system. *Am J Clin Pathol*. 1995; **104**(3): 279-82.